


Current Sensor BL12

Model BL12-60A-1.134VAC-60Hz

Serial 34485

External load of 400

Data taken on 02/15/01

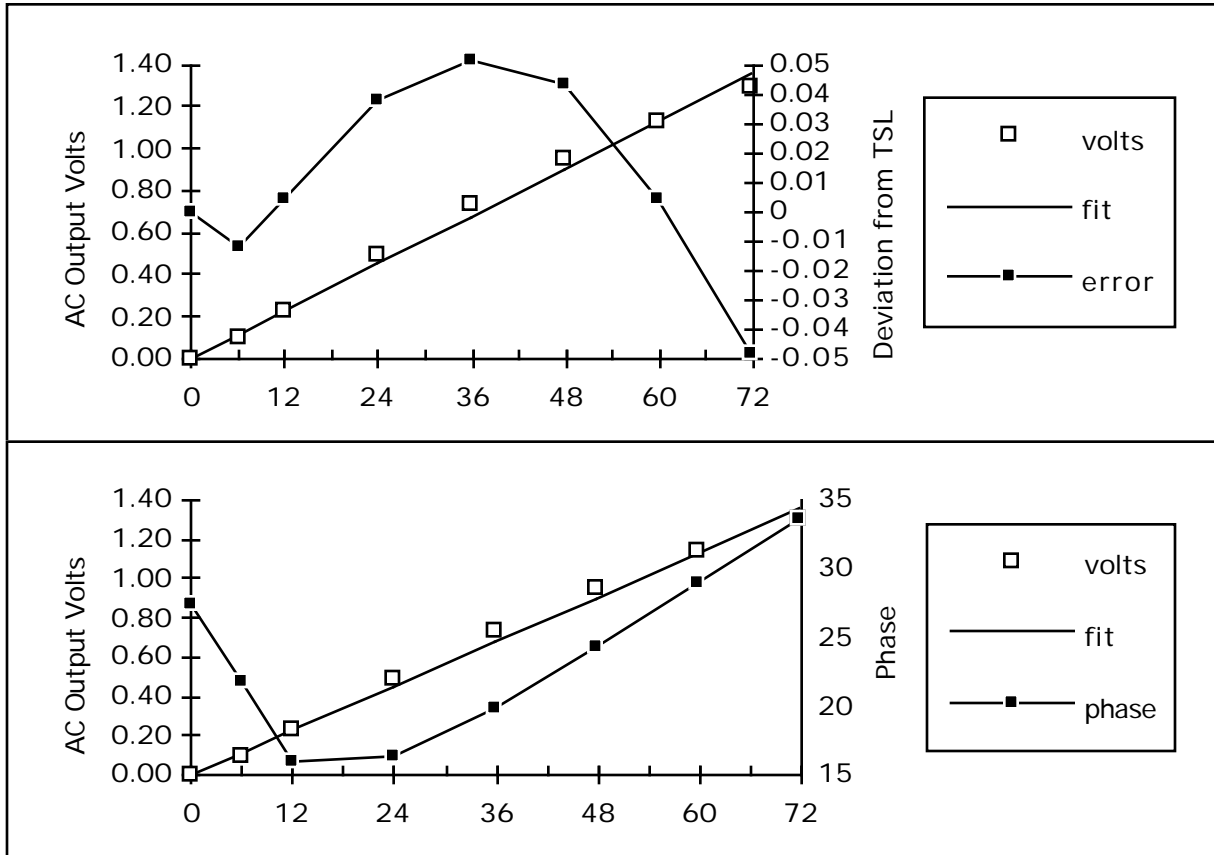

Amps	volts	fit	error	phase
0.00	0.00	0.00	0.0%	27.4
5.98	0.10	0.11	-1.2%	21.7
11.94	0.23	0.23	0.4%	16.0
23.88	0.49	0.45	3.8%	16.4
35.84	0.74	0.68	5.2%	19.9
47.76	0.95	0.90	4.3%	24.3
59.72	1.13	1.13	0.5%	29.0
71.64	1.30	1.35	-4.8%	33.7

Smith Research & Technology, Inc.



3109 N. Cascade Ave., Bldg. #201
 Colorado Springs, CO 80907-5190
 719 634 2259, FAX 719 634 2601