
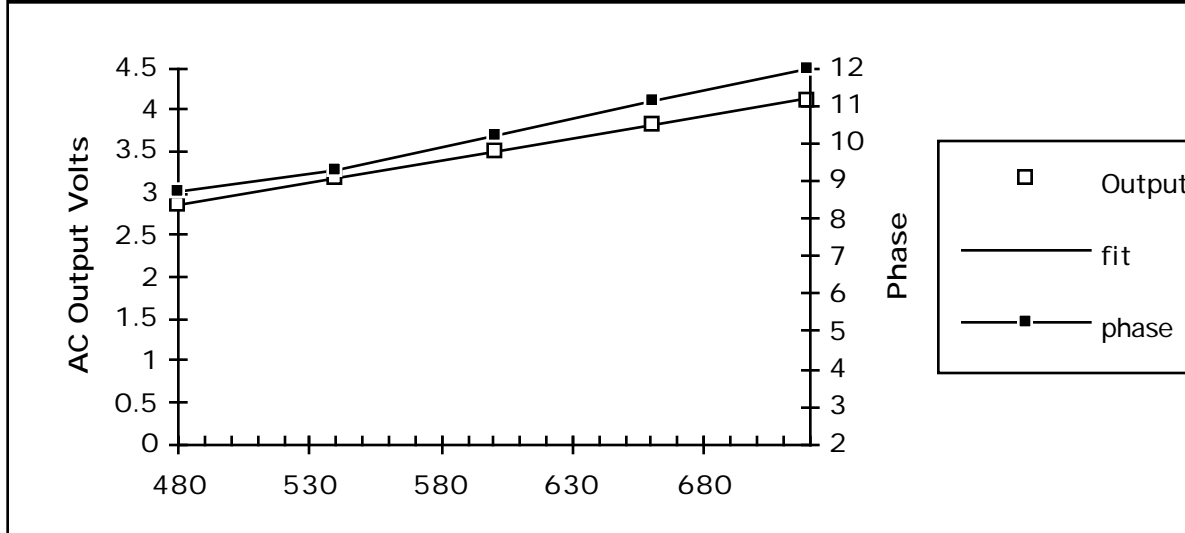


AC-output voltage sensor

Model VDO600MB-3.5VAC-60Hz
 Serial 940728-6
 Data taken on 07/30/94

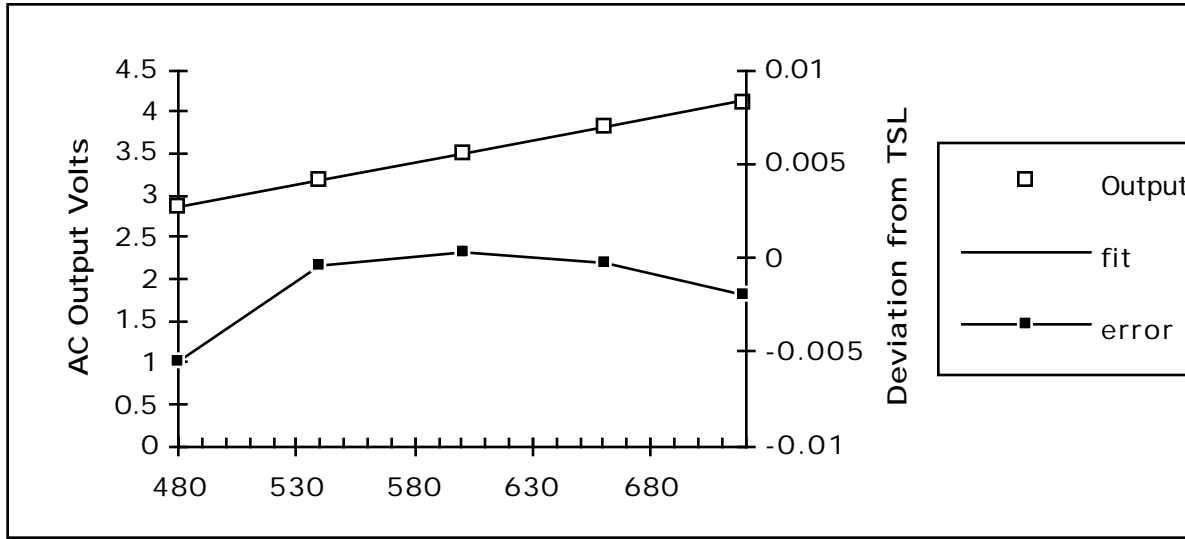


Input volts	Output volts	fit	error	phase
480.10	2.85	2.87	-0.01	8.70
540.20	3.18	3.18	0.00	9.30
600.20	3.50	3.50	0.00	10.20
660.30	3.82	3.82	0.00	11.10
719.90	4.11	4.13	0.00	12.00
156.00	4.45	4.48	0.00	8.20

Smith Research & Technolog



3109 N. Cascade Ave., Bldg
 Colorado Springs, CO 809
 719 634 2259, FAX 719 634 2258

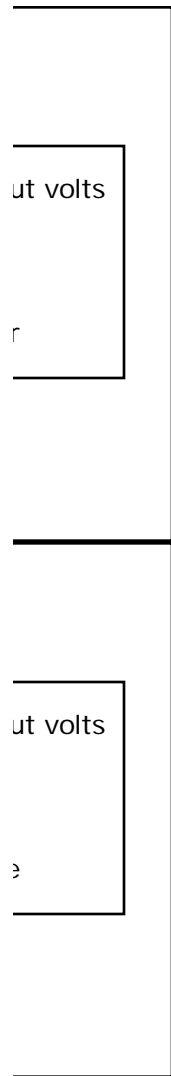

ogy, Inc.
Bldg. #201
0907-5190
) 634 2601